

ASPEC® 271: Automated Extraction of Aflatoxin M₁ from Milk



APPLICATION NOTE 1009

APPLICATION BENEFITS

Analytical testing is crucial for maintaining food safety. Successful detection of toxins, such as Aflatoxin M₁, in dairy products requires reliable and reproducible pre-analytical sample preparation. Food testing labs need reliable automated methods that standardize sample handling and free skilled personnel for more valuable tasks.

SOLUTIONS

Automation of methods for immunoaffinity cleanup and HPLC analysis provides precise quantification of toxins. Gilson's ASPEC® 271 system and TRILUTION® LH Software deliver easy-to-use method development, with the flexibility meet changing needs in the food testing laboratory. Aflatoxin M₁ was recovered from milk samples with repeatability and reproducibility in compliance with AOAC method 2000.08.

RAFAEL VON SPERLING DE SOUZA, FABIANO NARCISO PASCHOAL, EDUARDO BIECKEL, DANIELA DE AZEVEDO SILVA & MARIZE SILVA DE OLIVEIRA | Laboratory for Mycotoxin Analysis of the Ezequiel Dias Research Foundation; Belo Horizonte, MG, Brazil

ABSTRACT

Aflatoxin M₁, the main hepatic metabolic product of Aflatoxin B₁, was isolated from milk samples using the ASPEC® 271 system with excellent recovery, repeatability, and reproducibility. Automation of AOAC Method 2000.08 with the ASPEC 271 system provided a reliable, hands-off solution for the detection of this potentially carcinogenic food supply contaminant.

INTRODUCTION

Aspergillus is both one of the most useful and most harmful fungal genera known. Some species, including *A. niger* and *A. oryzae*, are critical to industrial fermentation processes,¹ while others produce toxic and secondary carcinogenic metabolites known as aflatoxins.

Aflatoxins are mycotoxins produced by fungi of the genus *Aspergillus*, principally the species *A. flavus* and *A. parasiticus*. Aflatoxins are found as contaminants in a variety of staple commodities, including grains, maize, and peanuts. These compounds are quite stable and can survive relatively high temperatures, including pasteurization² and the milk fermentation process,³ and are known to cause liver damage, reproductive effects, and immune suppression. The major aflatoxin species are B₁, B₂, G₁, and G₂ with Aflatoxin B₁ being the most toxic. The two main metabolic products, M₁ (refer to [Figure 2](#)) and M₂, are produced in the liver



Figure 1
ASPEC® 271 with VERITY® 4020 Single Syringe Pump




Figure 2
Chemical structure of Aflatoxin M₁, CAS No. 6795-23-9

from B₁ and B₂, respectively. Aflatoxin M₁ is a Group 2B carcinogen (possibly carcinogenic to humans) present in the milk of lactating mammals that ingest food contaminated with aflatoxin B₁.⁴

The World Health Organization (WHO), Food and Agriculture Organization of the United Nations (FAO), U.S. Department of Agriculture (USDA), and U.S. Food and Drug Administration (FDA), among other organizations, categorize aflatoxin as a serious health risk and have established maximum levels for the occurrence of this toxin in food products. Food testing laboratories face the challenge of meeting regulatory requirements and implementing reliable and reproducible methods for identification of toxins and other hazards in order to ensure a safe food supply.

The Association of Official Analytical Chemists (AOAC) has established a method for detection of Aflatoxin M₁ in milk.^{5,6} This method incorporates sample cleanup using an immunoaffinity column and analytical chromatography with fluorometric detection. Sample preparation by this method requires many steps carried out in a precise fashion. A Gilson automated solid phase extraction cartridge (ASPEC) liquid handler was used to automate the sample preparation and cleanup method.

In this application note we examine the limits of quantification and detection, repeatability, reproducibility, and recovery. Automation with the ASPEC 271 system provides a reproducible and reliable method for the isolation of Aflatoxin M₁ from milk samples using AOAC Official Method 2000.08.

MATERIALS AND METHODS

Samples and Reagents

Reagents and chemicals were ACS grade quality or better. Aflatoxin M₁ standard was obtained from Sigma-Aldrich® (PN A6428). HPLC-grade acetonitrile was obtained from Panreac AppliChem (PN 361881). All water was purified using a Milli-Q® system or equivalent.

Preparation of Sample Prior to SPE

Milk samples were heated at 37 ± 2°C and centrifuged for 15 minutes at 4000 rpm (2800 x g). After centrifugation, the upper fat layer was discarded and the sample was filtered with filter paper before being transferred to a 50 mL Falcon tube on the bed of the ASPEC 271.

METHODS

SOLID PHASE EXTRACTION	
Instrumentation	ASPEC 271
Cartridge	VICAM® Afla M ₁ ™ HPLC
Load	50 mL pre-treated sample at 1.5 mL/min
Wash	20 mL water at 3 mL/min; air push of 24 mL at 40 mL/min
Elute	2 mL acetonitrile at 1 mL/min
Elute	2 mL acetonitrile at 1 mL/min; 20 mL air push at 40 mL/min

Solid phase extraction was automated using a ASPEC 271 controlled with Gilson TRILUTION LH. Afla M₁ HPLC cartridges from VICAM® (PN G1007) were used for affinity purification of Aflatoxin M₁ as follows: 50 mL of pre-treated milk was loaded onto a cartridge at a flow rate of 1.5 mL/min. Cartridges were washed with 20 mL of water at 3 mL/min, followed by an air push (24 mL at 40 mL/min flow rate). Two rounds of elution were carried out, each with 2 mL acetonitrile applied at 1 mL/min. This was followed by an air push (20 mL air at 40 mL/min flow rate). The 4 mL of collected extract was evaporated to dryness in a water bath at 50°C under a gentle stream of nitrogen. The dry extract was then dissolved in 500 µL of mobile phase (water/acetonitrile, 67:33, v/v), filtered through a syringe filter of modified PTFE membrane, and frozen until HPLC analysis.

HPLC	
Instrumentation	Shimadzu HPLC Prominence®: System Controller CBM-20A System with fluorescence detection Degassing Unit DGU-20A5 Solvent Delivery Unit LC-20AT Autosampler SIL-10AF Column Oven CTO-20A Fluorescence Detector RF-20A
Column	Shimadzu® RP C18, 5 µm, 250 x 4.6 mm (Shimadzu® PN 228-34937-92) Shimadzu® C18 guard column, 5 µm, 10.0 x 4.0 mm (Shimadzu® PN 228-34938-91)
Gradient	Water/Acetonitrile 67:33; 1.0 mL/min
Injection Volume	50 µL
Detection	Fluorescence detection; excitation/emission: 365/435 nm

RESULTS AND DISCUSSION

Sample cleanup and extraction of Aflatoxin M₁ from milk samples was automated using the ASPEC 271 system. Immunoaffinity cartridges (Afla M₁ HPLC cartridges from VICAM®) were placed in a Gilson DEC rack, a mobile rack that is used for automated solid phase extraction. The ASPEC 271 can automatically load, condition, and wash the column, followed by eluting the compound(s) of interest. The automated procedure is diagrammed in [Figure 3](#).

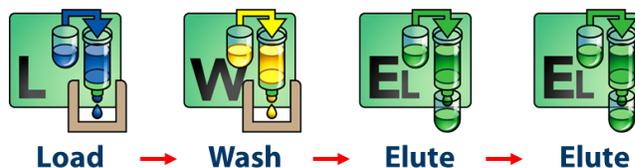


Figure 3
Schematic of the SPE process in TRILUTION® LH Software

Repeatability, Reproducibility, and Recovery

Repeatability, reproducibility, and recovery were assessed from the results obtained by two different analysts on two different days. Analysis by HPLC was performed in triplicate with three replicate samples at three different concentration levels. A representative HPLC trace is shown in [Figure 4](#).

A summary of the results of the repeatability, reproducibility, and recovery study is presented in [Table 1](#). These values are in agreement with the published relative standard deviation numbers from the AOAC formal collaborative studies.⁷

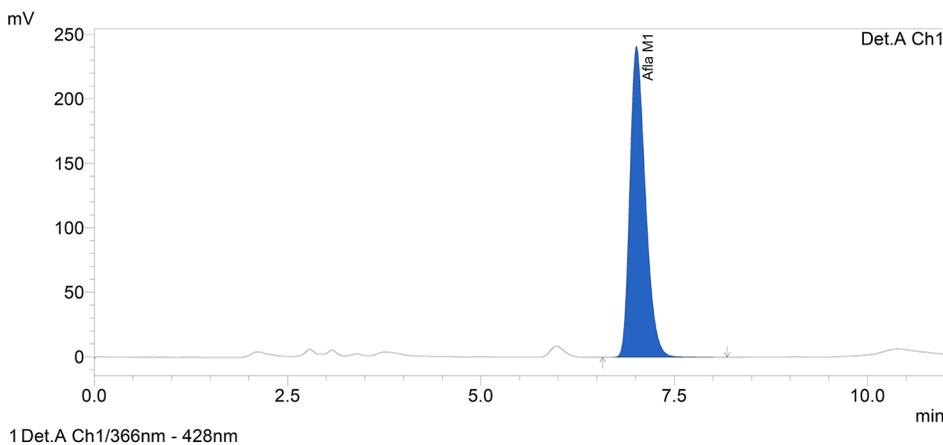


Figure 4
Representative HPLC chromatogram from this study with an Aflatoxin M₁ peak at ~7 minutes.

Table 1

Repeatability, reproducibility, and recovery values for Aflatoxin M₁

CONCENTRATION (µg/L)	REPEATABILITY RSD _R , (%)	REPRODUCIBILITY RSD _R , (%)	RECOVERY (%)
0.12	13.42	13.42	110
0.40	7.62	12.47	104
0.70	7.83	7.83	107

Detection and Quantification Limits

The limit of detection was determined to be three times the standard deviation of the intercept divided by the slope from the calibration curve used in the linearity assessment. The limit of quantification was taken as the lowest point of the linear range of the method.⁸

Table 2

Detection and quantification limits for Aflatoxin M₁.

AFLATOXIN M ₁	
Limit of Detection (µg/L)	0.02
Limit of Quantification (µg/L)	0.12

CONCLUSIONS AND BENEFITS

While ELISA-based techniques can permit easy detection of the presence of mycotoxins, the methods are subject to false positive results. Analysis by HPLC after cleanup with immunoaffinity columns is therefore required for precise quantitation of the toxins. The chromatographic methods require extensive sample preparation steps and well-trained personnel. This application note shows the advantage of automating sample cleanup using the ASPEC 271:

- Precise and reproducible loading of large volume samples (50 mL)
- Compatibility with commonly used labware (Falcon tubes)
- Multiple elution steps to improve recovery
- Unattended sample preparation frees skilled personnel for more valuable tasks
- Recovery, repeatability, and reproducibility in accordance with AOAC Official Method 2000.08

The ASPEC 271 is compatible not only with Gilson's pre-capped Silica, C18, SCX, WCX, HLB and other SPE cartridges, but also with all 1 mL, 3 mL and 6 mL commercial cartridges, and can therefore be used for any solid phase extraction procedures in the laboratory.

REFERENCES

1. Volk, T. "[Tom Volk's Fungus of the Month for February 1997.](#)" 1997. Accessed 13 June 2016.
2. Awasthi V, Bahman S, Thakur LK, Singh SK, Dua A, Ganguly S. Contaminants in milk and impact of heating: An assessment study. *Indian J Public Health*, 56, 95-99 (2012).
3. Lawley, R. "[Food Safety Watch: Aflatoxins.](#)" 2013. Accessed 14 June 2016
4. Desjardins, AE et al. Mycotoxins: risks in plant, animal, and humans systems. Task Council for Agricultural Science and Technology, Ames, Iowa, USA.
5. AOAC Official Method 2000.08. Aflatoxin M₁ in liquid milk, immunoaffinity column by liquid chromatography. Natural Toxins-chapter 49 (pp. 45-47). Official Methods of Analysis of AOAC International, 18th edition, AOAC International. Gaithersburg, Maryland 20877-2417, USA. (2005)
6. Dragacci S, Grosso F, Gilbert J., *Journal of AOAC International*, Immunoaffinity Column Cleanup with Liquid Chromatography for Determination of Aflatoxin M₁ in Liquid Milk: Collaborative Study, 84 (2) 437-443.
7. Thompson M, Ellison SLR, Wood R. Harmonized guidelines for single-laboratory validation of methods of analysis. *Pure and Applied Chemistry*, 74, 835-855 (2002).
8. Saini SS, Kaur A, The Analysis of Aflatoxin M₁ in Dairy Products. *Separation Science*, 5(10), 8-18. www.sepscience.com.

ACKNOWLEDGEMENTS

The authors thank Nova Analítica for the technical support provided in the development of this work.

Trademarks

All product and company names are trademarks™ or registered® trademarks of their respective holders. Use of the trademark(s) in this document does not imply any affiliation with or endorsement by the trademark holder(s).